

1 Disintegration Test Accessories




101-2000 Depth and stroke calibration gauge (certificate optional)



101-2240 USP/EP standard basket: (PTZE, PTZAUTO)
105-2240 (PTZ-S, DIST3)




101-2148-6 standard disintegration USP/EP Disks

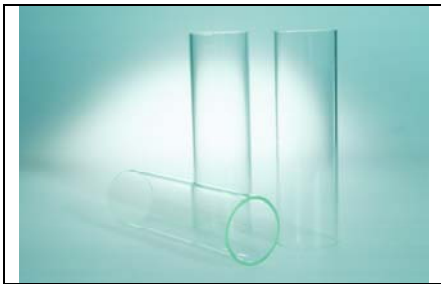


101-2145-6 USP/EP standard glass




12-20100 PT-MKT Standard Auto Disintegration Basket
6 Testing Positions

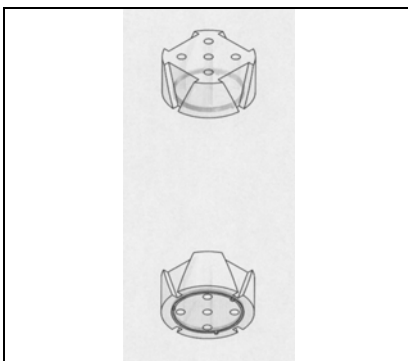

102-1020-6 PT-MK disks with metal contact ring and metal needles

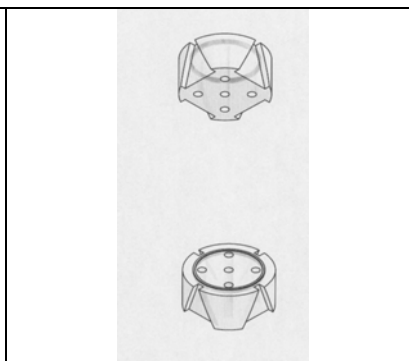

102-1015-6 PT-MK disks with metal ring (no needle)

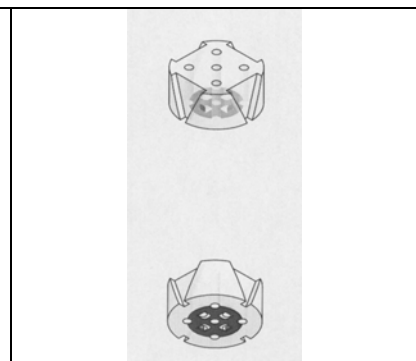

102-1005-6 PT-MK disks and metal contact plate


PHARMA TEST AG
Siemensstrasse 5
D-63512 Hainburg (GER)



+49 6182 9532-600
+49 6182 9532-650
email@pharma-test.de
www.pharma-test.com



2 Manual Disintegration Basket for bigger samples, up to 33 mm, in compliance to EP 2.9.1.2

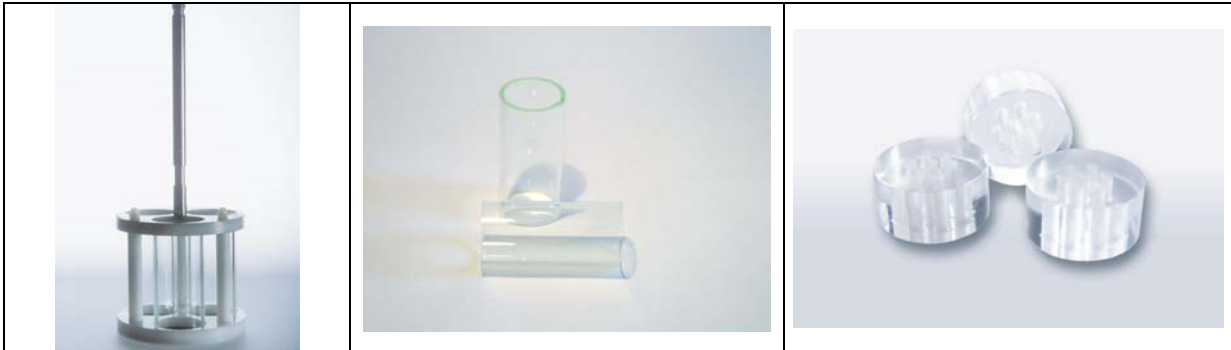


101-2014 Disintegration Basket (EP 2.9.1.2) 3 tubes for PTZE/PTZAUTO
105-2014 for PTZS/DIST3

101-2015-3 glass tubes 33mm

101-2016-3 Disks 33mm

3 Auto-Disintegration Test Basket with 3 tubes (EP 2.9.1.2)

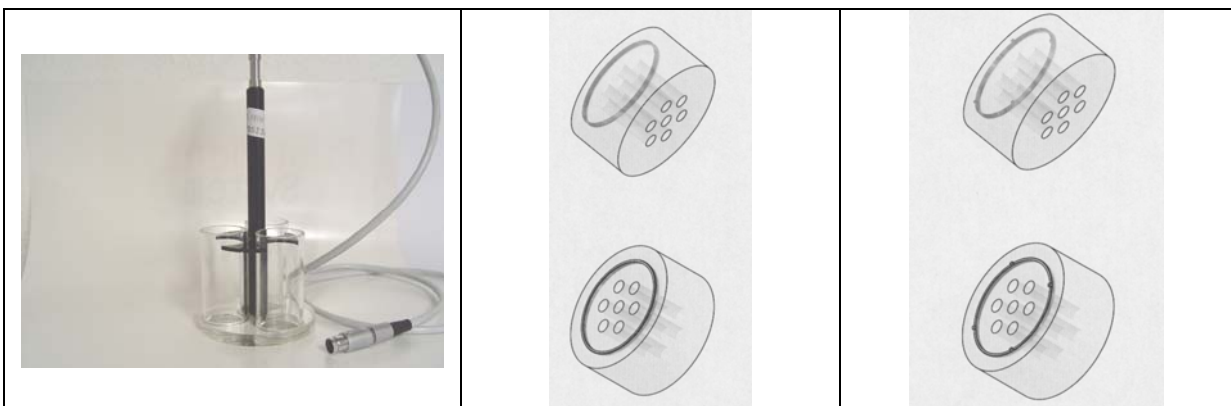

12-20200 PT-MK33 Auto Disintegration Basket (EP 2.9.1.2)

102-1115-3 PT-MK33 Disk with metal ring, no needle

102-1120-3 PT-MK33 Disk with 3 metal ring and needles